




Somos la empresa líder en las líneas de productos, equipamientos y soluciones de gestión hospitalaria (HIS-RIS-PACS).

SANTO DOMINGO

Máximo Avilés Blonda No. 37,
Ens. Julieta, Santo Domingo
República Dominicana

809.620.8660
info@unique.com.do

PRODUCTOS DE PREVENCIÓN COVID-19

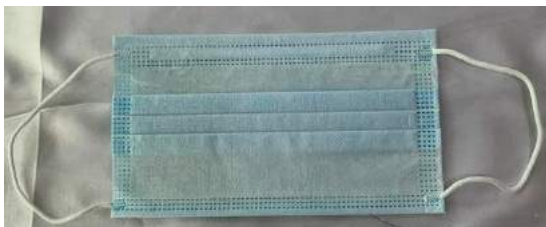

Tamaño: 175mm*95mm

Material: PP no tejido

Color: Azul

Empaque: 50 Und./Paq.-Caja,
40 Paq.-Caja/Cartón, 2000 und/Ctn.

Tamaño de cartón: 50*40*30cm/Ctn


CBM/Ctn: 0,06

Peso: 7,7 kg

Certificados: CE, FDA, Test Report


Cantidad mínima: 40,000 und.

CERTIFICADOS

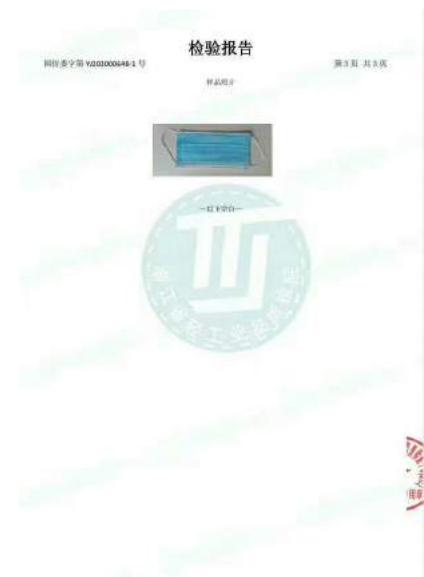

MASCARILLA

Mascarila KN95 Desechable Sin Válvula, Para Uso Civil

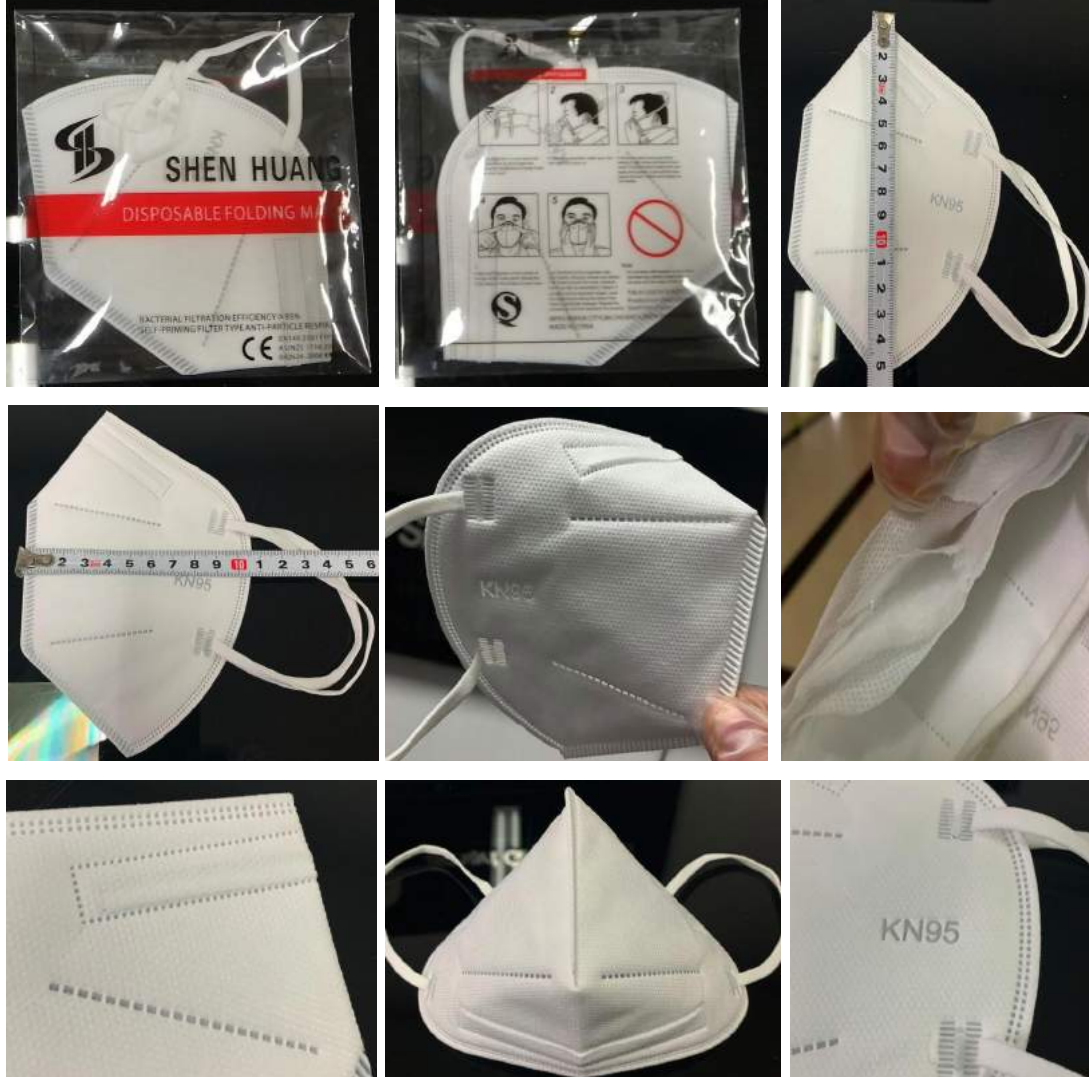

4 Capas

Material: PP no tejido, tejido fundido,
capa de esponja

Efecto de filtrado: $\geq 95\%$

Color: Blanco

Empaque: 1 und./Paq - 1,000 Paq/Cartón

Tamaño de cartón: 50*45*35cm

CBM/Ctn: 0,08

Peso/Ctn: 9,6 kg

Certificados: CE ENG149: 2001 + A1 2009,
FFP2 NRD TYPE IIR, JC 9501
GB-2626:2006, Test Report

Cantidad mínima: 10,000 unidades

PRODUCTOS DE PREVENCIÓN COVID-19 CERTIFICADOS

ECM Certificate – 證明書 – Certificate – 증명서

Form ECM_1, 2014, version 03, official use document

Certificate of Compliance

No. 42/2023/29.1.2.03.03

Certificate's
Holder:

Jinhua jinhua labor protection tool
factory
No. 103 Linhu Street, Tangxi town, Jinhua City

Certificate ECM
Mark:

Product:
Model(s):
Verification lot:

shenhuang
J2004JC9901JC9902JC9903
Stands
EN 149: 2001 A1 2009

related to CE Declaration(s)
R 2014/525 (Personal Protective Equipment)

Remark: This document has been issued on a voluntary basis and upon request of the manufacturer. It is to confirm that the technical documentation submitted from the manufacturer is suitable for the requirements of the ECM Initiative. The conformity mark above cannot affect the product's conformity to the ECM requirement for its use.

Additional information and feedback are welcome.

The manufacturer is responsible for the CE marking process, and it remains valid only in a limited way. This document has been issued on the basis of the information on ECM Initiative data for the verification of products. ECM won't investigate it.

Issuance date: 29 March 2023
expiry date: 30 March 2025

Use the Certificate Machine V1
 Visit our Website: 240 - Link: Contacts at Newsletter - <ECS@consumerlab.com> <ECS@consumerlab.com>
 ✉ <ECS@consumerlab.com> <ECS@consumerlab.com> <ECS@consumerlab.com> <ECS@consumerlab.com>

[illegible]

Proprietary Name	Product Codes	Device Class	Listing Number	Establishment Operations
Diyswaki Prosthetic Mask (P301, P3562, P3006, Steel Jaw)	A5T1	II	P342099	Manufacturer

END OF THE ANNEX



For use by: **FAIR (Pharm) Certification Co., Ltd.**

excise director

Dated: March 30, 2020

FAIR (pharm) Certification Co., Ltd. Tel: 02-0260551 E-Mail: fair@fair.co.th
 Website: www.fair.co.th Mail: 261-001, No. 1 Lane 191, Tsinghai Road, Huayung District, Bangkok, Thailand, 10110

合格证	
QUALIFIED CERTIFICATE	
公司名称 COMPANY	金华市金创劳动防护用品厂
公司地址 COMPANY ADD	中国浙江省金华市金东区孝顺镇新街村1155号一幢一樓 Jinhua City 321017 Zhejiang Province, China
电话 TEL	0579-82665689 0579-82665689
品名 PRODUCT NAME	口罩 mask
规格 PRODUCT SPEC	11x15.5 11x15.5
执行标准 PRODUCT STANDARD	GB2626-2006KN95 GB2626-2006 KN95
生产日期 MANUFACTURING DATE	2020.4月 04-2020
失效日期 EXPIRING DATE	2023.4月 04-2023

PRODUCT DESCRIPTION AND CERTIFICATION

SHENHUANG SAFE + MASK FF NR D



CLASS II MEDICAL DEVICE

English instructions for safe disposal and pre-use type are stipulated separately
本產品之安全處理及預用說明書分別列明
中文說明書一併附於產品包裝盒內，請用戶注意說明書

ENGLISH

English Instruction
Concentrations and evaluation represent evaluation according to test reports
• FFH, FFH NR D are disposable masks, classified as Class II Medical Tools (MD). They are available for personal protection.

Warning for medical professionals
• Disposable masks and other medical devices are also classified as Class II Medical Tools (MD). They are available for medical personnel, physicians, and hospital visitors.
FFH, FFH NR D include the following points:

- Protection against aerosol (aerosol) or airborne liquid or solid particles (existing in the air-respiratory diseases)
- Protect local and distant infectious bacteria and viruses.

The manufacturer refers to accept responsibility for damage caused by failure to follow the instructions below.
Because the mask may differ in Figure 1, 2, 3 & 4.

This mask can only be used by trained people.

Remove the mask from the packaging bag before using it immediately.

After use, make sure the mask is **folded** on the face, then throw it away (Figure 5)
Do not bend over the mask. Block the surface on each side, possible, and do not move the mask.

Always store the mask in a cool, dry place, do not use and avoid the expired date.

- If there is use in the hand of the nose area, please adjust the mask that from the nose area (see Figure 4)
- If there is a crease in the nose part of the mask, carefully adjust the crease.

If the mask is not tight enough, do not enter service it is needed. Please choose a different type of mask and make sure it is tight enough.

Please use:

- Do you feel dizzy or vertigo or any pain.
- Feeling trouble (sneezing)
- Rashness and itchy skin.
- Mouth dryness
- Moisture appears you have breathing
- Compromised by blood or other liquids.

If such a situation occurs, dispose of the mask through the normal channel of the infectious disease hazard unit.

The mask can be simply used like Figure 7. As the performance of the mask will decrease, repeated use of the mask can cause damage to the face and the device on the helmet is surrounding people.

Precautions:
The mask cannot prevent fog or white film formation.
This mask does not prevent fogging. Please use it in an environment with at least 12% oxygen.
Do not use in negative atmospheric.

Precautions:
• (1) Conventional respiratory use.
• Minimum concentration: see Figure 11

Storage:
According to the recommendations displayed on the package Storage: See Figures 3-10


After 2 years after production date
Distribution as required

Disclaimer:
Accident investigation: Any serious problem caused by the use of the product should be notified to the manufacturer and local authorities.


PRODUCT DESCRIPTION AND CERTIFICATION

SHENHUANG SAFE + MASK N95 NR D


English and instructions for using disposable self protecting filter type and particulate respirator
 产品说明：一次性自保护式过滤式防颗粒物呼吸器使用指南




1




2




3




4




5




6




7



8







9



10

	FIT NR D	FFP2 NR D	FFP3 NR D
	4.5 VME	10.5 VME	20.5 VME
English: Sensation: 0.001 (0.001) - 5000 + A1 - 5000 中文: 感觉: 0.001 (0.001) - A1 - 5000 中文: 检测灵敏度: 0.001 (0.001) + 5000			
	43050	43055	03100
English: Efficiency < 95% 中文: 效率 < 95% (0.05-2000)	Efficiency efficiency 95%	Efficiency efficiency 95%	Efficiency efficiency < 95.0%
English: Sensation: 0.001 (0.001) - 5000 + A1 - 5000 中文: 感觉: 0.001 (0.001) - 5000 中文: 检测灵敏度: 0.001 (0.001) - 5000			

CHINA LABOR PROTECTION PRODUCTS QUALITY SUPERVISION AND INSPECTION CENTER(BEIJING)

SHENHUANG SAFE + MASK N95 INSPECTION REPORT

Sample name	Self priming filter type anti particle respirator	Sample company	Jinchuang
Specifications	Disposable mask	Protective level	KN95
Requester name	Jishua city Jinchuang Labor Protection Tool Factory	Requester contact details	Goldsmack @163.com
Requester address	Jishua china		
Production unit name	Jishua city Jinchuang Labor Protection Tool Factory	manufacturer contact details	Goldsmack @163.com
Manufacturer Address	Jishua china		
Number of samples	10	Production Date	————
Sample status	unused	Post date	04.02.2020
Sample Characteristics	White labbing mask	Send samples	Jinchuang
Test based on	GB 2626-2006. (Respiratory protection Self priming filter type anti-particle respirator)		
Test items	Filtration efficiency, Inhalation resistance, Expiratory resistance		
Test results	<p>Samples tested According to GB 2626-2006. (Respiratory protection Self priming filter type anti-particle respirator) It is determined that the test data meets KN95 standard requirements.</p> <p>Issued: February 20, 2020</p>		
Notes	Samples are not preserved		
Ready:	陈泽方	Check:	尹超
		Main aspects:	周志华

SECTION REPORT NUMBER: 20190925-010				New arrival																			
1	100% 100% 100%	English This page reports the requirements defined below in Japanese and in English. (中) に記載された日本語を優先し ます。英文と日本語が合致しない 場合は、日本語が優先されます。	English The evaluation results are as follows. 日本語 評価結果は以下のとおり です。		English evaluation results are as follows. 日本語 評価結果は以下の ようです。																		
			<table border="1"> <thead> <tr> <th>Passing (Evaluation sufficient)</th> <th>Fail (Evaluation insufficient)</th> </tr> </thead> <tbody> <tr> <td>15</td> <td>85.25</td> </tr> <tr> <td>20</td> <td>86.25</td> </tr> <tr> <td>25</td> <td>88.25</td> </tr> <tr> <td>30</td> <td>89.25</td> </tr> <tr> <td>35</td> <td>91.25</td> </tr> <tr> <td>40</td> <td>93.25</td> </tr> <tr> <td>45</td> <td>95.25</td> </tr> <tr> <td>50</td> <td>96.25</td> </tr> <tr> <td>55</td> <td>98.25</td> </tr> <tr> <td>60</td> <td>99.25</td> </tr> </tbody> </table>	Passing (Evaluation sufficient)		Fail (Evaluation insufficient)	15	85.25	20	86.25	25	88.25	30	89.25	35	91.25	40	93.25	45	95.25	50	96.25	55
Passing (Evaluation sufficient)	Fail (Evaluation insufficient)																						
15	85.25																						
20	86.25																						
25	88.25																						
30	89.25																						
35	91.25																						
40	93.25																						
45	95.25																						
50	96.25																						
55	98.25																						
60	99.25																						
2	80.0 80.0 80.0	English This page reports the requirements defined below in Japanese and in English. (中) に記載された日本語を優先し ます。英文と日本語が合致しない 場合は、日本語が優先されます。	English The evaluation results are as follows. 日本語 評価結果は以下のとおり です。		English evaluation results are as follows. 日本語 評価結果は以下の ようです。																		
			<table border="1"> <thead> <tr> <th>Passing (Evaluation sufficient)</th> <th>Fail (Evaluation insufficient)</th> </tr> </thead> <tbody> <tr> <td>15</td> <td>85.25</td> </tr> <tr> <td>20</td> <td>86.25</td> </tr> <tr> <td>25</td> <td>88.25</td> </tr> <tr> <td>30</td> <td>89.25</td> </tr> <tr> <td>35</td> <td>91.25</td> </tr> <tr> <td>40</td> <td>93.25</td> </tr> <tr> <td>45</td> <td>95.25</td> </tr> <tr> <td>50</td> <td>96.25</td> </tr> <tr> <td>55</td> <td>98.25</td> </tr> <tr> <td>60</td> <td>99.25</td> </tr> </tbody> </table>	Passing (Evaluation sufficient)		Fail (Evaluation insufficient)	15	85.25	20	86.25	25	88.25	30	89.25	35	91.25	40	93.25	45	95.25	50	96.25	55
Passing (Evaluation sufficient)	Fail (Evaluation insufficient)																						
15	85.25																						
20	86.25																						
25	88.25																						
30	89.25																						
35	91.25																						
40	93.25																						
45	95.25																						
50	96.25																						
55	98.25																						
60	99.25																						
3	80.0 80.0 80.0	English This page reports the requirements defined below in Japanese and in English. (中) に記載された日本語を優先し ます。英文と日本語が合致しない 場合は、日本語が優先されます。	English The evaluation results are as follows. 日本語 評価結果は以下のとおり です。		English evaluation results are as follows. 日本語 評価結果は以下の ようです。																		
			<table border="1"> <thead> <tr> <th>Passing (Evaluation sufficient)</th> <th>Fail (Evaluation insufficient)</th> </tr> </thead> <tbody> <tr> <td>15</td> <td>85.25</td> </tr> <tr> <td>20</td> <td>86.25</td> </tr> <tr> <td>25</td> <td>88.25</td> </tr> <tr> <td>30</td> <td>89.25</td> </tr> <tr> <td>35</td> <td>91.25</td> </tr> <tr> <td>40</td> <td>93.25</td> </tr> <tr> <td>45</td> <td>95.25</td> </tr> <tr> <td>50</td> <td>96.25</td> </tr> <tr> <td>55</td> <td>98.25</td> </tr> <tr> <td>60</td> <td>99.25</td> </tr> </tbody> </table>	Passing (Evaluation sufficient)		Fail (Evaluation insufficient)	15	85.25	20	86.25	25	88.25	30	89.25	35	91.25	40	93.25	45	95.25	50	96.25	55
Passing (Evaluation sufficient)	Fail (Evaluation insufficient)																						
15	85.25																						
20	86.25																						
25	88.25																						
30	89.25																						
35	91.25																						
40	93.25																						
45	95.25																						
50	96.25																						
55	98.25																						
60	99.25																						
4	80.0 80.0 80.0	English This page reports the requirements defined below in Japanese and in English. (中) に記載された日本語を優先し ます。英文と日本語が合致しない 場合は、日本語が優先されます。	English The evaluation results are as follows. 日本語 評価結果は以下のとおり です。		English evaluation results are as follows. 日本語 評価結果は以下の ようです。																		
			<table border="1"> <thead> <tr> <th>Passing (Evaluation sufficient)</th> <th>Fail (Evaluation insufficient)</th> </tr> </thead> <tbody> <tr> <td>15</td> <td>85.25</td> </tr> <tr> <td>20</td> <td>86.25</td> </tr> <tr> <td>25</td> <td>88.25</td> </tr> <tr> <td>30</td> <td>89.25</td> </tr> <tr> <td>35</td> <td>91.25</td> </tr> <tr> <td>40</td> <td>93.25</td> </tr> <tr> <td>45</td> <td>95.25</td> </tr> <tr> <td>50</td> <td>96.25</td> </tr> <tr> <td>55</td> <td>98.25</td> </tr> <tr> <td>60</td> <td>99.25</td> </tr> </tbody> </table>	Passing (Evaluation sufficient)		Fail (Evaluation insufficient)	15	85.25	20	86.25	25	88.25	30	89.25	35	91.25	40	93.25	45	95.25	50	96.25	55
Passing (Evaluation sufficient)	Fail (Evaluation insufficient)																						
15	85.25																						
20	86.25																						
25	88.25																						
30	89.25																						
35	91.25																						
40	93.25																						
45	95.25																						
50	96.25																						
55	98.25																						
60	99.25																						
5	80.0 80.0 80.0	English This page reports the requirements defined below in Japanese and in English. (中) に記載された日本語を優先し ます。英文と日本語が合致しない 場合は、日本語が優先されます。	English The evaluation results are as follows. 日本語 評価結果は以下のとおり です。		English evaluation results are as follows. 日本語 評価結果は以下の ようです。																		
			<table border="1"> <thead> <tr> <th>Passing (Evaluation sufficient)</th> <th>Fail (Evaluation insufficient)</th> </tr> </thead> <tbody> <tr> <td>15</td> <td>85.25</td> </tr> <tr> <td>20</td> <td>86.25</td> </tr> <tr> <td>25</td> <td>88.25</td> </tr> <tr> <td>30</td> <td>89.25</td> </tr> <tr> <td>35</td> <td>91.25</td> </tr> <tr> <td>40</td> <td>93.25</td> </tr> <tr> <td>45</td> <td>95.25</td> </tr> <tr> <td>50</td> <td>96.25</td> </tr> <tr> <td>55</td> <td>98.25</td> </tr> <tr> <td>60</td> <td>99.25</td> </tr> </tbody> </table>	Passing (Evaluation sufficient)		Fail (Evaluation insufficient)	15	85.25	20	86.25	25	88.25	30	89.25	35	91.25	40	93.25	45	95.25	50	96.25	55
Passing (Evaluation sufficient)	Fail (Evaluation insufficient)																						
15	85.25																						
20	86.25																						
25	88.25																						
30	89.25																						
35	91.25																						
40	93.25																						
45	95.25																						
50	96.25																						
55	98.25																						
60	99.25																						
6	80.0 80.0 80.0	English This page reports the requirements defined below in Japanese and in English. (中) に記載された日本語を優先し ます。英文と日本語が合致しない 場合は、日本語が優先されます。	English The evaluation results are as follows. 日本語 評価結果は以下のとおり です。		English evaluation results are as follows. 日本語 評価結果は以下の ようです。																		
			<table border="1"> <thead> <tr> <th>Passing (Evaluation sufficient)</th> <th>Fail (Evaluation insufficient)</th> </tr> </thead> <tbody> <tr> <td>15</td> <td>85.25</td> </tr> <tr> <td>20</td> <td>86.25</td> </tr> <tr> <td>25</td> <td>88.25</td> </tr> <tr> <td>30</td> <td>89.25</td> </tr> <tr> <td>35</td> <td>91.25</td> </tr> <tr> <td>40</td> <td>93.25</td> </tr> <tr> <td>45</td> <td>95.25</td> </tr> <tr> <td>50</td> <td>96.25</td> </tr> <tr> <td>55</td> <td>98.25</td> </tr> <tr> <td>60</td> <td>99.25</td> </tr> </tbody> </table>	Passing (Evaluation sufficient)		Fail (Evaluation insufficient)	15	85.25	20	86.25	25	88.25	30	89.25	35	91.25	40	93.25	45	95.25	50	96.25	55
Passing (Evaluation sufficient)	Fail (Evaluation insufficient)																						
15	85.25																						
20	86.25																						
25	88.25																						
30	89.25																						
35	91.25																						
40	93.25																						
45	95.25																						
50	96.25																						
55	98.25																						
60	99.25																						
7	80.0 80.0 80.0	English This page reports the requirements defined below in Japanese and in English. (中) に記載された日本語を優先し ます。英文と日本語が合致しない 場合は、日本語が優先されます。	English The evaluation results are as follows. 日本語 評価結果は以下のとおり です。		English evaluation results are as follows. 日本語 評価結果は以下の ようです。																		
			<table border="1"> <thead> <tr> <th>Passing (Evaluation sufficient)</th> <th>Fail (Evaluation insufficient)</th> </tr> </thead> <tbody> <tr> <td>15</td> <td>85.25</td> </tr> <tr> <td>20</td> <td>86.25</td> </tr> <tr> <td>25</td> <td>88.25</td> </tr> <tr> <td>30</td> <td>89.25</td> </tr> <tr> <td>35</td> <td>91.25</td> </tr> <tr> <td>40</td> <td>93.25</td> </tr> <tr> <td>45</td> <td>95.25</td></tr></tbody></table>	Passing (Evaluation sufficient)		Fail (Evaluation insufficient)	15	85.25	20	86.25	25	88.25	30	89.25	35	91.25	40	93.25	45	95.25			
Passing (Evaluation sufficient)	Fail (Evaluation insufficient)																						
15	85.25																						
20	86.25																						
25	88.25																						
30	89.25																						
35	91.25																						
40	93.25																						
45	95.25																						



Material: Material de lente PC

Color: Transparente

Transmitancia de luz: 98%

Empaque: 1 Und/Paq OPP, 10 unds Paq OPP/Caj
25 Cajas/Cartón - 250 unds/Cartón

Tamaño de cartón: 80*40*36cm

CBM/Ctn: 0,1152

Peso: 9,5 kg

Certificados: CE, FDA

Cantidad mínima: 2,000 unds

PRODUCTOS DE PREVENCIÓN COVID-19

TRAJE DE PROTECCIÓN MÉDICA

Traje de Protección Desechable



Beijing Winsunny Harmony Science & Technology Co., Ltd. File No. FH-CE-06 Edition: A/0

DECLARATION OF CONFORMITY TO COUNCIL DIRECTIVE 93/42/EEC CONCERNING MEDICAL DEVICES	
 MANUFACTURER:	Beijing Winsunny Harmony Science & Technology Co., Ltd. Guangyundongjie 88 4unit, Tongzhou District, Beijing, P.R.China. Building 9, 68 Guanghua Road, Zhangjiawan Town, Tongzhou District, Beijing, P.R.China.
MEDICAL DEVICE:	Disposable protective clothing against infective agents
SPECIFICATION:	FH-168/165/170/175/180/185/190/195
CLASSIFICATION - ANNEX IX:	Class I, Rule 1
CONFORMITY ASSESSMENT ROUTE:	MDD 93/42/EEC Annex VII
 EC REP	Shanghai International Holding Corp. GmbH (Europe) Eiffelstrasse 88, 20537 Hamburg, Germany Tel: +49-40-2513175, Fax: +49-40-255726
EUROPEAN REPRESENTATIVE:	
We, THE MANUFACTURER, HEREBY DECLARE THAT THE STATED MEDICAL DEVICE MEET THE TRANSPOSITION INTO NATIONAL LAW, THE PROVISIONS OF COUNCIL DIRECTIVE 93/42/EEC CONCERNING MEDICAL DEVICES; ALL SUPPORTING DOCUMENTATION IS RETAINED AT THE PREMISES OF THE MANUFACTURER, AND THE MANUFACTURER IS EXCLUSIVELY RESPONSIBLE FOR THE DECLARATION OF CONFORMITY.	
START OF CE-MARKING: 2020-3-17	
PLACE, DATE OF DECLARATION:	<BEIJING> 2020-3-16
SIGNATURE:	 NAME: MR. XUERUI LIU POSITION: GENERAL MANAGER

Sin cubrezapatos

No esterilizado

Empaque: 1 Traje/Paq, 25 Paq/Cartón

Tamaño de cartón: 78*49*30cm

CBM/Ctn: 0,1147

Certificado: CE

Cantidad mínima: 1,000 unds.

TERMÓMETRO

Termómetro Infrarojo AOV8810



Sonido de alerta

Modos duales

Memoria

Tamaño: 70*125mm

Unidad de peso: 100g

Empaque: 60 unds/cartón

CBM/Ctn: 0,086

Peso/Ctn: 11,5 kg

Certificados: CE, FDA

Cantidad mínima: 50 unds.

CERTIFICADOS



Con bolsillo transparente para identificación

Tamaño: 90x200cm

Material: PVC Eco-amigable 0.3mm

Color: Negro

Capacidad: 200 kgs

CBM/Ctn: 0,09

Certificados: CE, SGS

Cantidad mínima: 1,000 unds.

CERTIFICADOS

Test Report Sample photo:	No. CANM.2004350101	Date: 07 Apr 2020	Page 5 of 5
	<div style="text-align: center;">  <p>CANM.2004350101</p> <p>CANM-J00191.001</p> </div>		
300 authenticates the photo on original report only *** End of Report ***			



UYGUNLUK ONAYI

ATTESTATION OF COMPLIANCE



Applicant:

Manufacturer:

Product:

Type/Model:

DONDUKULU
T.1 Kurbanlar, Yedigöller Mahallesi, Kızıltepe İlçesi, Gaziantep
San. Ülk. San. B. İl. Gaziantep (City, Gaziantep Province, China)

DONDUKULU
T.1 Kurbanlar, Yedigöller Mahallesi, Kızıltepe İlçesi, Gaziantep
San. Ülk. San. B. İl. Gaziantep (City, Gaziantep Province, China)

PCV

911

ITS FACTORY

PRODUCTS FACTORY

Reference Document(s): Donduklulu T.1/95-50 (10442)

Reference Standard(s): IEC 60335-1:2013

Date of attestation: File of Technical Documentation

Issue Date: 05.05.2020 **Expiry Date:** 05.05.2025

Intertek hereby confirms that the presented file of technical documentation declares conformity of the above mentioned products with the technical requirements of Certificate 2019-105640, provided that the attestation has been issued as per company request. This attestation does not absolve the conformity obligation of the manufacturer to issue the Declaration of conformity.



Signature (Official)
INTERTÉK Gaziantep
ENF 001-2019-05-05-0000





SANTO DOMINGO

Máximo Avilés Blonda No. 37,
Ens. Julieta, Santo Domingo
República Dominicana

809.620.8660
info@unique.com.do